

Compact, Rugged, and Low-Cost Wavelength-Versatile Burst Laser (Army STTR)

Final Technical Report

April 18, 2013 to April 17, 2015

Proposal Number: A2-4987

Contract Number: W911NF-13-C-0050

Table of Contents

1. Project Objectives	Page 3
2. Work Performed	Page 4
2.1 Phase II Technical Objectives and Approach.	Page 4
2.2 Kickoff Meeting (May 2013)	Page 4
2.3 Year 1 Schedule	Page 5
2.4 Year 2 Schedule	Page 5
2.5 Laser System Concept	Page 5
2.6 Master Oscillator Power Amplifier (MOPA) Laser Configuration	Page 6
2.7 Diode Arrays for the New MOPA Configuration	Page 8
2.8 Q-Switched MO	Page 8
2.9 Power Amplifier (PA)	Page 10
2.10 MOPA Performance	Page 10
2.11 Wavelength Converters	Page 12
2.11.1 1570nm Converter	Page 12
2.11.2 355nm Converter	Page 13
2.11.3 266nm Converter	Page 14
2.12 Wavelength Separator	Page 16
2.13 Low Cost Design Considerations	Page 17
2.14 Compact Low Cost Laser Driver	Page 25
2.15 Low Cost Q-Switch Driver	Page 26
2.16 Battery / Inverter Pack	Page 26
2.17 Complete Systems	Page 28

3.	Manual	Page 29
4.	Cost Estimates	Page 29
5.	Results Obtained	Page 29
6.	Estimates of Technical Feasibility	Page 29

1. List of Illustrations

1.	Figure 1 – Block diagram of the burst laser system	Page 6
2.	Figure 2 – 4 pass Laser MOPA configuration	Page 6
3.	Figure 3 – 4 pass Laser MOPA layout.	Page 7
4.	Figure 4 – 4 pass Laser MOPA design (left), and photograph (right).	Page 7
5.	Figure 5 – 2 pass Laser MOPA configuration	Page 8
6.	Figure 6 – New high pulse energy Q-switched MO	Page 8
7.	Figure 7 – Q-switch MO 8ns FWHM temporal pulse	Page 9
8.	Figure 8 – Q-switch MO pulse energy	Page 9
9.	Figure 9 – Q-switch MO spatial beam profile	Page 9
10.	Figure 10 – Photograph of the PA laser head	Page 10
11.	Figure 11 – MOPA layout on the right with the wavelength converter, and the actual MOPA on the left without the wavelength converter	Page 11
12.	Figure 12 – 1064nm MOPA pulse energy versus laser diodes' drive current (left) and the temporal pulse (right)	Page 11
13.	Figure 13 – Spatial burn of the 1064nm MOPA pulse (4mm diameter and 50mJ/pulse)	Page 12
14.	Figure 14 – Eye safe OPO KTP converter and wavelength separator	Page 12
15.	Figure 15 – 1570nm converter pulse energy and temporal pulse	Page 13
16.	Figure 16 – 355nm converter set-up using SHG followed by a THG	Page 13
17.	Figure 17 – 355nm converter pulse energy temporal pulse (9ns)	Page 14
18.	Figure 18 – 266nm converter set-up using SHG followed by a FHG	Page 14
19.	Figure 19 – 266nm converter pulse energy and temporal pulse (10ns)	Page 15
20.	Figure 20 –SolidWorks model of display cases	Page 15
21.	Figure 21 – Dust proof storage enclosure for the various wavelength converters	Page 16
22.	Figure 22–PB Prism mount ideas	Page 16
23.	Figure 23– 3D printed model of PB rotating mount	Page 17
24.	Figure 24 – Pellin-Broca prism arrangement for the wavelength separation	Page 17
25.	Figure 25– CAD model of custom mounting	Page 18
26.	Figure 26– CAD model of case with grommets	Page 19
27.	Figure 27– 3D model	Page 19
28.	Figure 28– CAD model of breadboard and case assembly.	Page 20
29.	Figure 29– 2D CAD drawing of part to be fabricated	Page 20
30.	Figure 30 – Machined components	Page 21
31.	Figure 31– Anodized Parts assembled on breadboard	Page 21
32.	Figure 32 – Custom designed laser rod mount	Page 22
33.	Figure 33 – SolidWorks model of new system design	Page 22

34. Figure 34 – System layout mockup using 3D printed components.	Page 23
35. Figure 35 – Parts to be anodized.	Page 23
36. Figure 36 – Parts to be anodized.	Page 24
37. Figure 37 – Multiple boards populated with anodized parts	Page 24
38. Figure 38 –Populated with anodized parts mounted in enclosure.	Page 24
39. Figure 39 – Block diagram of the laser driver	Page 25
40. Figure 40 – Extremely compact and low cost laser driver (includes power supply, diode driver, and Q-switch trigger) and it's current pulse	Page 25
41. Figure 41 – Extremely compact and low cost Q-switch driver	Page 26
42. Figure 42 –SolidWorks model design for battery case insert	Page 27
43. Figure 43 –SolidWorks model assembly for battery case insert	Page 27
44. Figure 44 – Polymer Li-ion battery for powering the burst laser system	Page 27
45. Figure 45 – Complete laser system (laser module in center, laser driver on left, and wavelength converters on right)	Page 28
46. Figure 46 – Burst laser in a briefcase	Page 28
47. Figure 47 – Three completed prototype burst lasers in their briefcases	Page 29
48. Figure 48 – Operator manual for the prototype burst laser	Page 29

Project objectives

Many laser-based sensor technologies like Raman, Laser Induced Fluorescence (LIF), UV Laser Photo-Dissociation (UV-PD), and Laser Induced Breakdown Spectroscopy (LIBS) are being developed for close contact and standoff threat chemical, biological, radiological, nuclear and explosives (CBRNE) analysis. These operate in a burst laser mode with a finite number of laser pulses required for the measurement. This is because either the sample/target is chemically altered with repeated laser shots, or the technique limits the number of shots for rapid sensor response.

The typical pulsed lasers currently used in these systems are Commercial off the Shelf (COTS) systems that have been designed for continuous operation for many hours. Therefore, these lasers are over engineered with regards to size, weight, cooling capacity, and cost.

Currently the most affordable pulsed laser systems are flashlamp pumped. However, diode pumped lasers are more desirable due to ruggedness, higher efficiency, and smaller size. So far, the Diode Pumped Solid State (DPSS) lasers have cost significantly more than flashlamp pumped lasers.

Our STTR project has the goal of producing DPSS burst laser that is (1) high pulse energy in a rapid burst mode, (2) wavelength agile to cover the eye-safer regions in the UV and near-IR, as well as (3) smaller, lighter, and much more affordable than current COTS systems.

Phase I started on August 31, 2011 and ended on February 28, 2012. Although the Phase I requirement was to produce an engineering model for the burst laser, we have taken it much further and built a breadboard demonstrator and successfully demonstrated its performance.

Burst Laser Goal Requirements:

- 50mJ/pulse @ 1064nm
- 5 - 10ns pulse duration
- <3xDL (Diffraction Limited) beam quality
- Other wavelengths options of 1.5 μ m and 355nm
- Up to 100 pulses burst
- <100Hz repetition rate (10Hz is sufficient)
- <1 minute between bursts
- <33% of current laser size (<850 cubic inch)
- <25% of current laser weight (<8.5lbs.)
- <33% of current laser cost (<\$8,500)

In Phase II (April 18, 2013 to April 17, 2015) our goal was to engineer, design and construct three prototype burst laser systems that show the feasibility of producing such lasers while meeting all of the above goal requirements.

Work Performed and Results Obtained

Phase II Technical Objectives and Approach


The technical objective of Phase II is to build and test three low cost prototype burst lasers that meet all the US Army requirements.

The approach to reach the above objective is by performing the following tasks: 1) design, fabrication, components procurement, assembly and testing of first prototype laser system based on Phase I effort, 2) incorporate new low cost diode arrays and address minor modifications if needed in updated design, then fabricate, procure components, assemble and test the next two prototype lasers and upgrade the first laser to the latest design.


Kickoff Meeting (May 2013)

The Phase II program started with a kickoff meeting that included the US Army representatives. Planned actions were described, followed by an open discussion on any deviations from the intended plan.

Year 1 Schedule

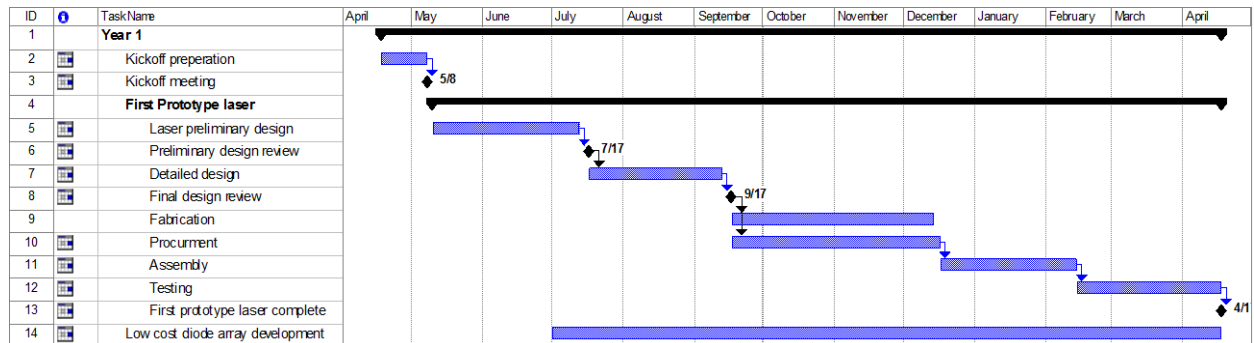

Year 2 Schedule

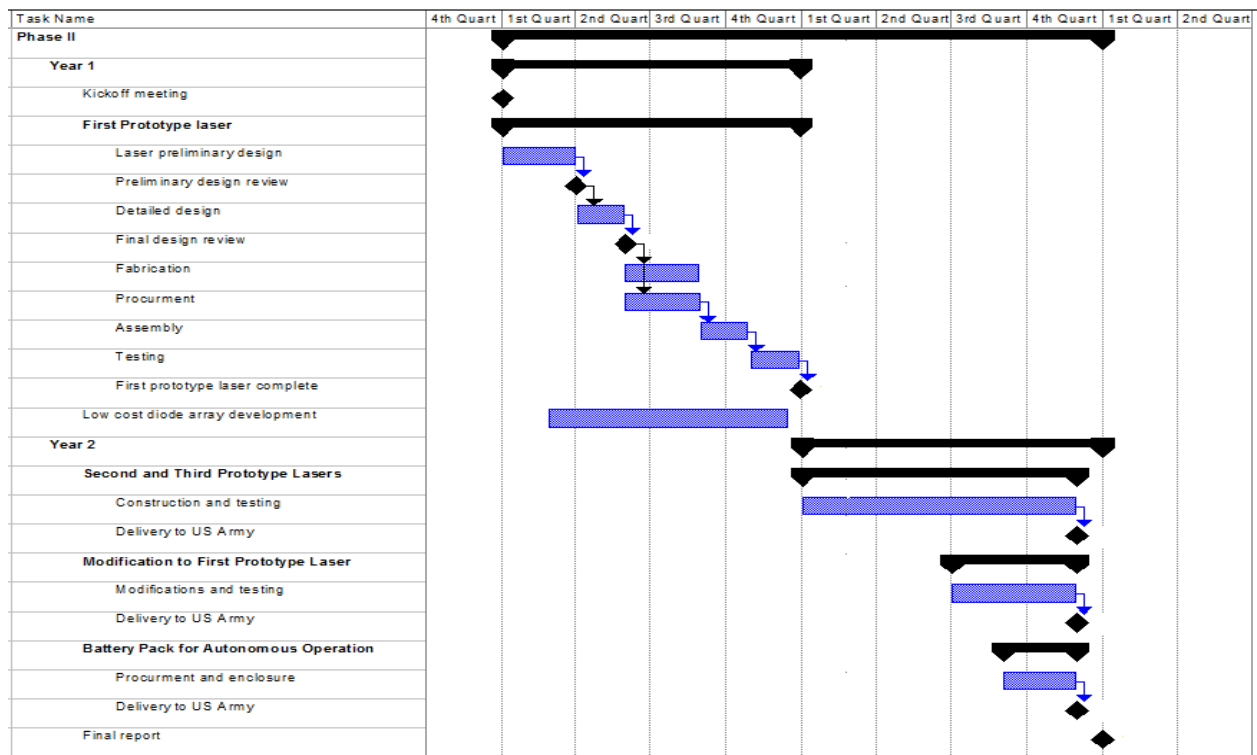

Laser System Concept

The laser system under development in Phase II is intended for both in house and field applications. It is designed to be used with a standard wall plug of 115Vac or with a 12Vdc and 115Vac inverter as shown in figure 1.

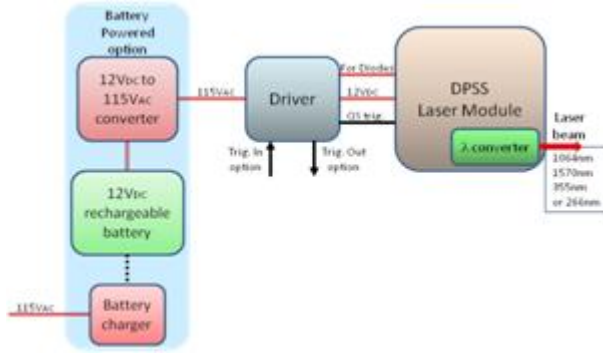


Figure 1 – Block diagram of the burst laser system

The Diode Pumped Solid State (DPSS) laser module produces 50mJ per pulse at 1064nm. The wavelength can be converted to 1570nm, 355nm or 266nm via the wavelength converters. The laser drive electronics is a separate module connected via a cord to enable more flexibility of operation. The laser driver plugs to 115Vac and has trigger IN and trigger OUT for synchronizing it with other detection equipment. For field application, a 12Vdc battery and inverter to 115Vac is provided. It can be hooked to a car battery with inverter or the provided battery pack.

Master Oscillator Power Amplifier (MOPA) Laser Configuration

Lasers that are used for LIBS and other optical based detections like LIF, Raman, etc. are simple laser oscillator design and flash lamp pumped for low cost. Operating a simple laser oscillator at high energy per pulse requires a trade-off between energy per pulse and beam quality. Higher energy per pulse translates to lower beam quality. We have chosen to go with diode pumped MOPA laser configuration for high performance. For this proposed burst laser we want high beam quality to allow for generating micro-plasma for LIBS at large standoff distance, and also for improved performance of the wavelength converters.

Figure 2 shows our 4 pass Master Oscillator Power Amplifier (MOPA) laser configuration.

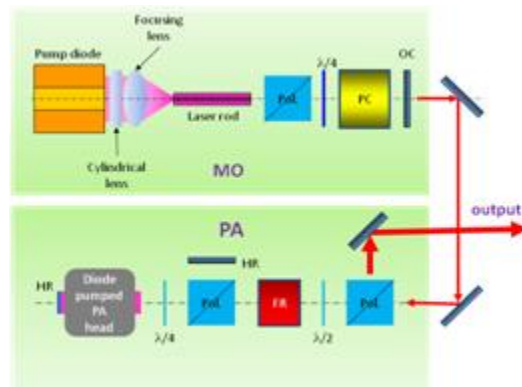


Figure 2 – 4 pass Laser MOPA configuration

The Master Oscillator (MO) is a longitudinally pumped Q-switched Nd:YAG laser. The pump diode build up the population inversion in the Nd:YAG rod during the pump duration of about $200\mu\text{s}$. The polarizer and the quarter waveplate prevent any lasing until the Pockels cell activates and undoes the quarter waveplate to allow lasing. The laser light escapes the resonator through the output coupler (OC). In this configuration, the pulse duration depends on the gain and the resonator length. The Power Amplifier (PA) is a passive four pass amplifier that boosts up the energy per pulse without affecting the beam properties.

In Year 1 of Phase II we constructed and tested the 4 pass MOPA laser. Figure 3 shows the layout of the laser.

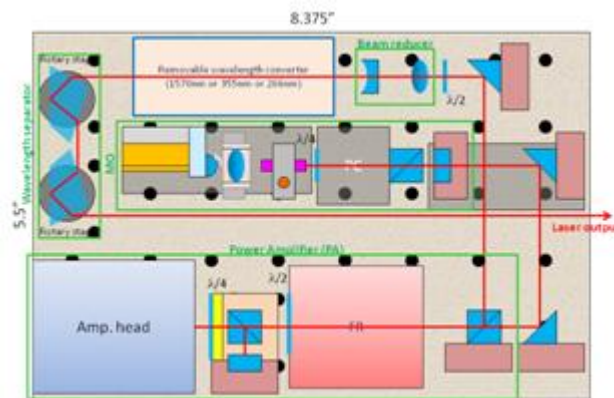


Figure 3 – 4 pass Laser MOPA layout

Figure 4 shows the design and a photograph of the 4 pass laser.

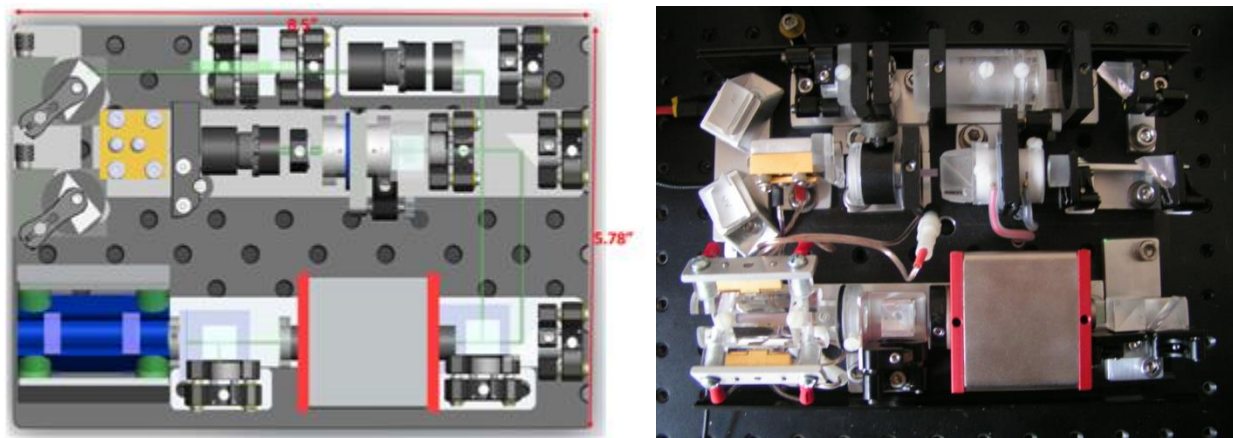


Figure 4 – 4 pass Laser MOPA design (left), and photograph (right)

By designing the laser for small size it was more difficult to get the laser to reach its desired performance. In addition, the high cost and weight of the Faraday rotator was a concern. In order to reduce the cost and weight, we modified the design. We increased the power out of the

Master Oscillator (MO) and changed the Power Amplifier (PA) configuration to 2 passes as shown in Figure 5.

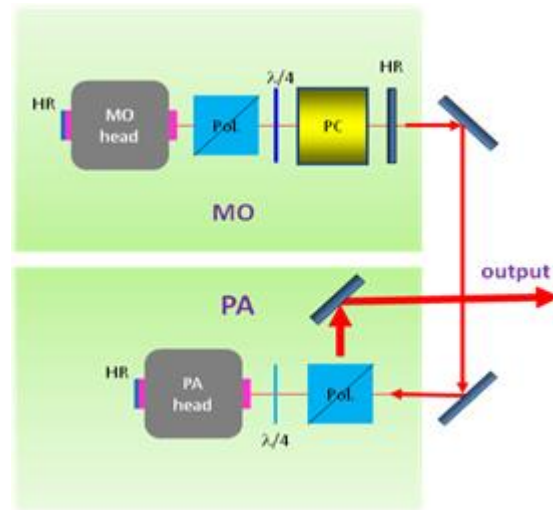


Figure 5 – 2 pass Laser MOPA configuration

Diode Arrays for the New MOPA Configuration

Diode arrays are the major cost components of the laser. We selected low duty cycle diode arrays with no cooling. The diode arrays were tested using 100 pulse bursts. The red shift of the arrays was $\sim 1.5\text{nm}$ which is within the required range of 3nm . We observed the wavelength shift live using a real time spectrometer.

Q-Switched MO

The new MOPA configuration requires higher energy per pulse in order to achieve the 50mJ output after only two pass amplification. We modified the MO design to have higher pump power and larger laser rod. A laser diode array is transversely pumping a 4mm diameter rod.

Figure 6 shows the MO that we designed and constructed.



Figure 6 – New high pulse energy Q-switched MO

This MO delivers $\sim 15\text{mJ}$ per pulse and 8 to 10 ns pulse duration.

Figure 7 shows the MO temporal pulse.

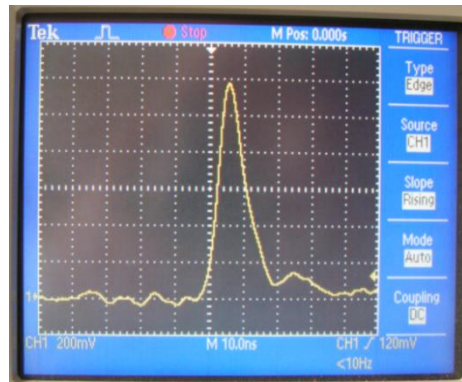


Figure 7 – Q-switch MO 8ns FWHM temporal pulse

Figure 8 shows the MO output pulse energy versus the drive current the diode array.

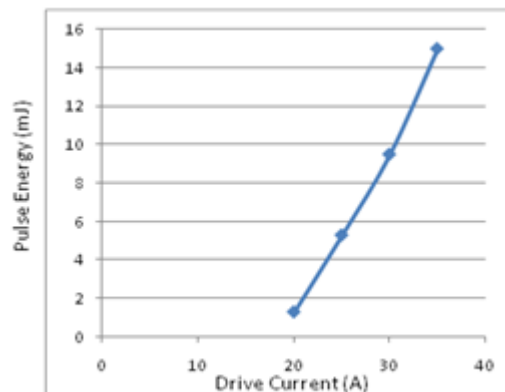


Figure 8 – Q-switch MO pulse energy

Figure 9 shows the spatial beam profile. The slight elongation is due to the pump array, but the beam is nearly diffraction limited and Gaussian in profile.

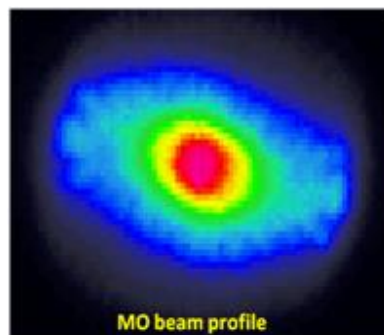


Figure 9 – Q-switch MO spatial beam profile

Power Amplifier (PA)

Burst mode operation is different than a typical laser operation. A typical solid state laser must run at a constant loading to maintain steady thermal conditions. Solid state lasers change their performance as components change their temperature. Laser diodes undergo red wavelength shift at elevated temperature, the laser crystals and harmonics generation crystals start lensing and the thermal stress induce birefringence. All this change need to be compensated to avoid laser performance degradation. Burst mode operation takes the laser components from low temperature to elevated temperature during the burst duration. In this case we have to ensure that the laser components will be within the range of acceptable performance.

The PA was designed and fabricated completely in house. It consists of a single diode array that transversely pumps a 4mm Nd:YAG laser rod. A photograph of the PA laser head is shown in figure 10.

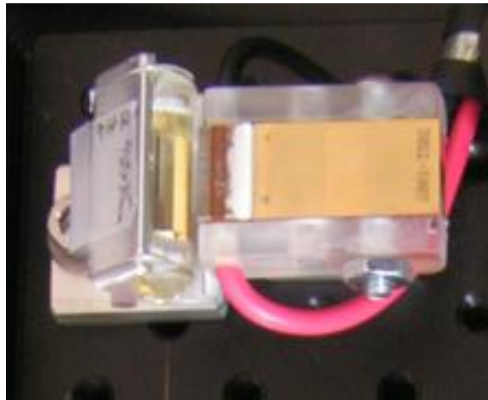


Figure 10 – Photograph of the PA laser head

MOPA Performance

The MOPA layout is shown in figure 11.

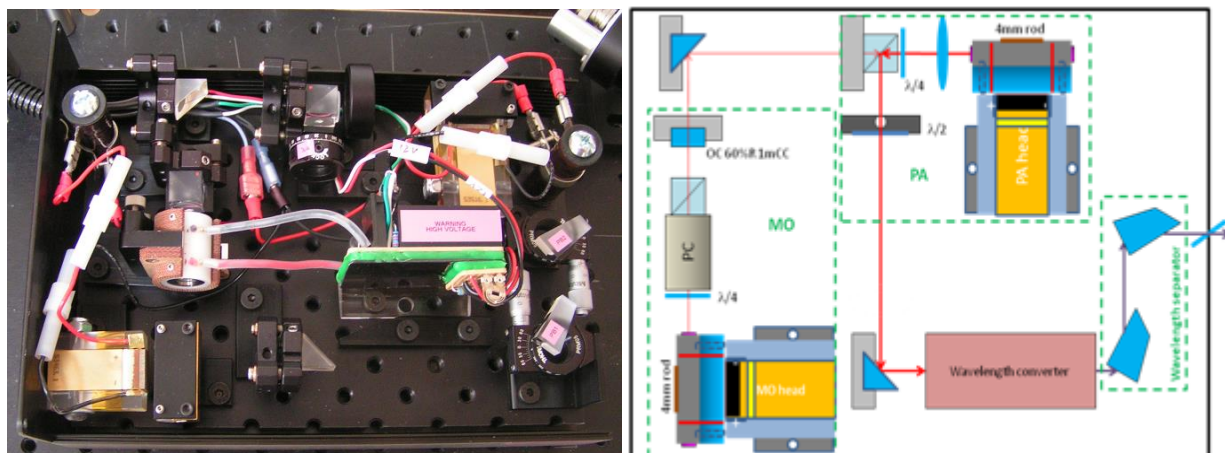


Figure 11 – MOPA layout on the right with the wavelength converter, and the actual MOPA on the left without the wavelength converter

The MOPA pulse energy and temporal pulse are shown in figure 12. The FWHM was between 8ns to 10ns for the various burst lasers constructed.

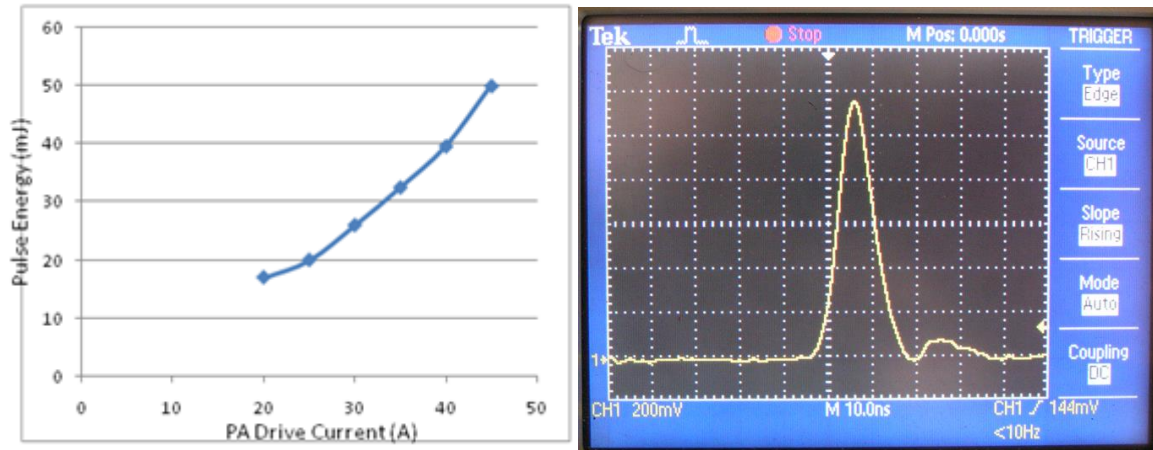


Figure 12 – 1064nm MOPA pulse energy versus laser diodes' drive current (left) and the temporal pulse (right)

Figure 13 is the burn pattern of the MOPA output pulse.

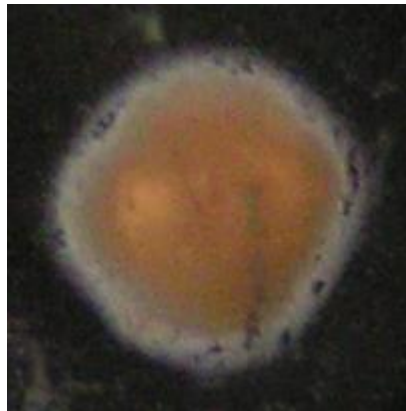


Figure 13 – Spatial burn of the 1064nm MOPA pulse (4mm diameter and 50mJ/pulse)

Wavelength Converters

The laser system has the option to generate other wavelengths of interest by converting the fundamental wavelength of 1064nm.

1570nm Converter

For safe operation in the field, it is a standard practice to use eye safe wavelength like 1.5 μ m. There are several techniques for shifting the fundamental to longer wavelengths. The most elegant, efficient and compact is by using OPO (Optical Parametric Oscillator). The set-up for the converter is shown in figure 14.

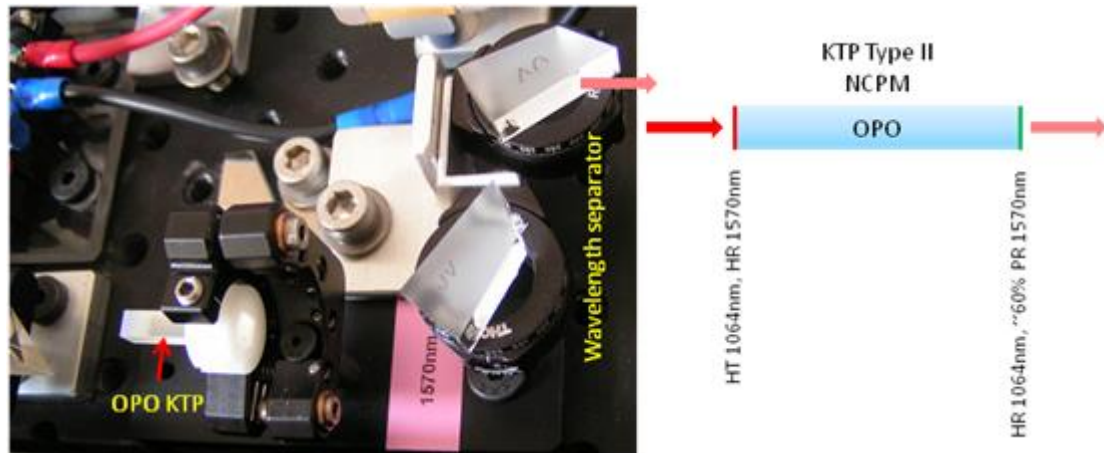


Figure 14 – Eye safe OPO KTP converter and wavelength separator

The optical coatings are done on the crystal itself in order to reduce size and cost.

We obtained pulse energy of about 3.3mJ at 1570nm, and pulse duration of 10ns as shown in figure 15.

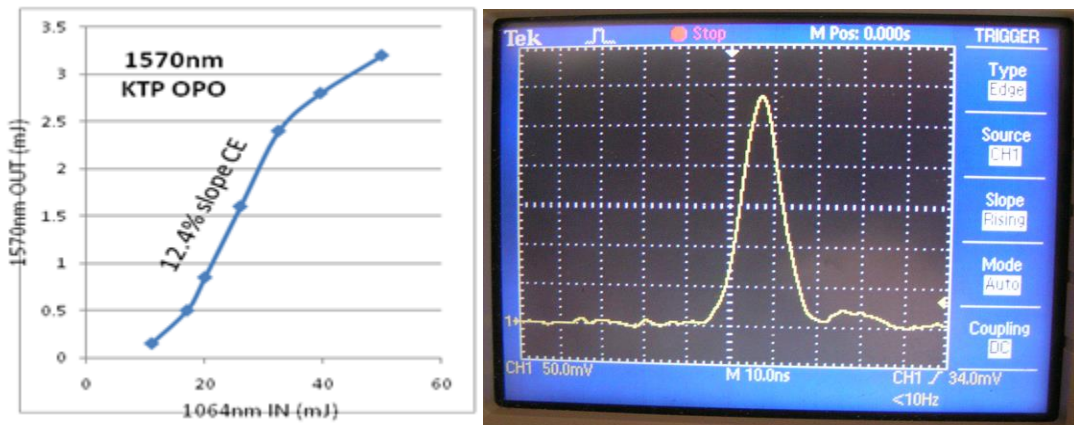


Figure 15 – 1570nm converter pulse energy and temporal pulse

355nm Converter

The set-up for generating the third harmonics of 355nm is shown in figure 16.

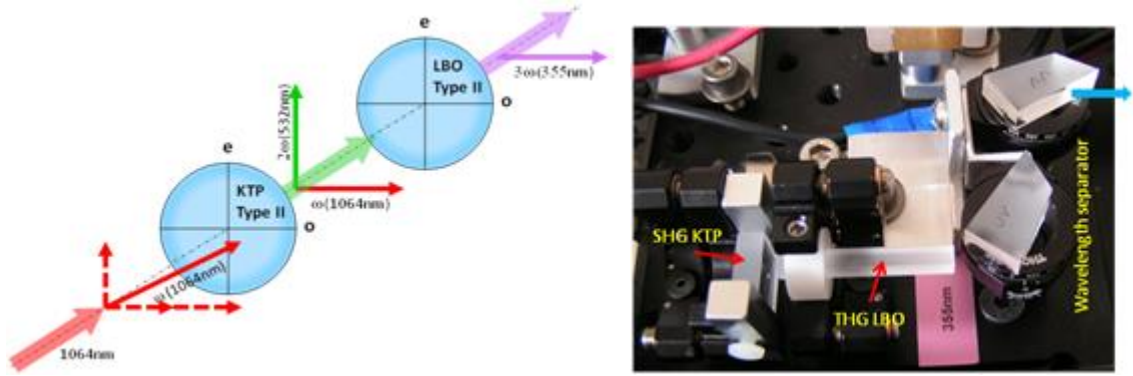


Figure 16 – 355nm converter set-up using SHG followed by a THG

The wavelength separation is done via the two Pellin-Broca prisms. We obtained up to 6mJ/pulse in the third harmonics.

Figure 17 shows the pulse energy and the temporal pulse of the third harmonics.

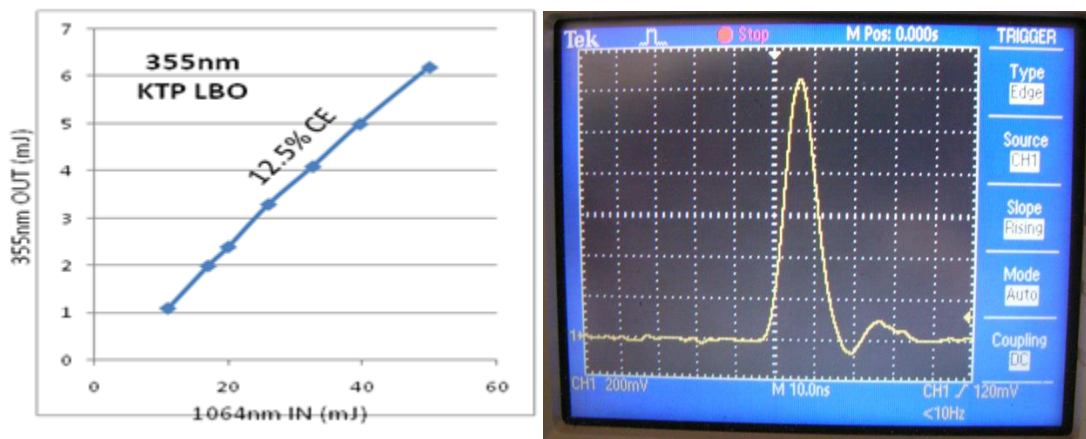


Figure 17 – 355nm converter pulse energy temporal pulse (9ns)

266nm Converter

The set-up for generating the third harmonics of 355nm is shown in figure 18.

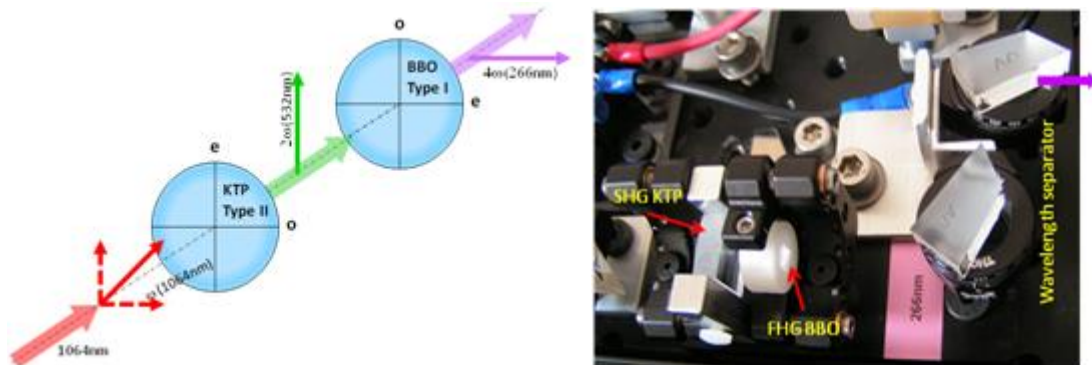


Figure 18 – 266nm converter set-up using SHG followed by a FHG

The wavelength separation is done via the two Pellin-Broca prisms. We obtained up to 1.5mJ/pulse in the fourth harmonics.

Figure 19 shows the pulse energy and the temporal pulse of the fourth harmonics.

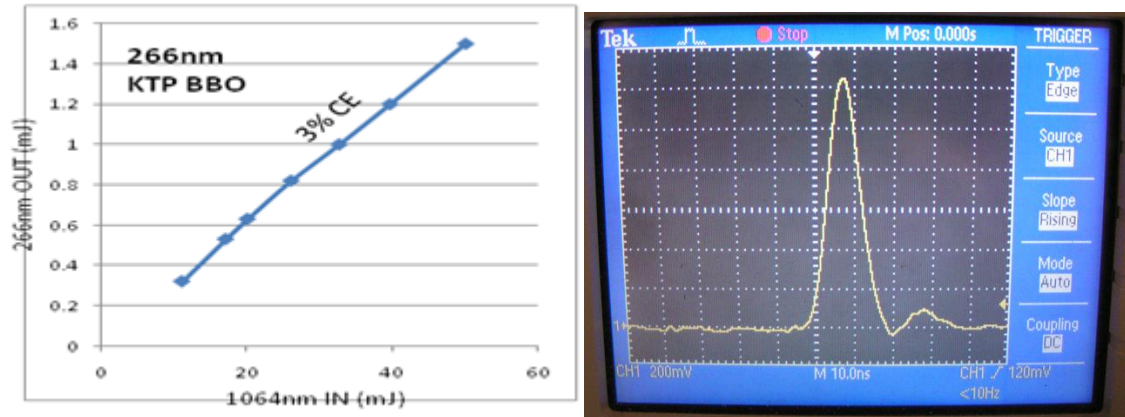


Figure 19– 266nm converter pulse energy and temporal pulse (10ns)

Display cases for keeping the unused wavelength converters dust free were designed and fabricated (Figure 20)

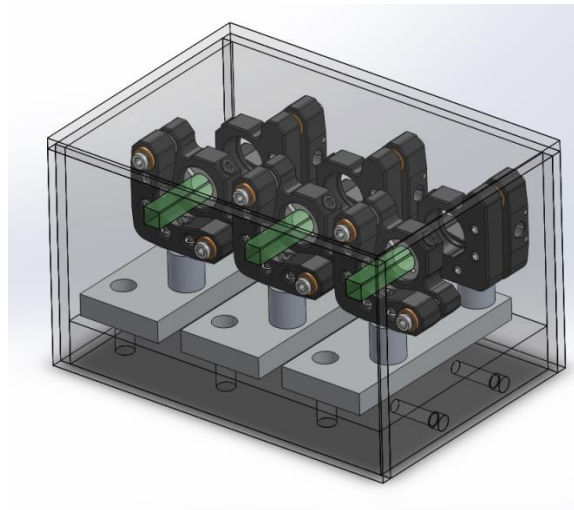


Figure 20 –SolidWorks model of display cases

Figure 21 shows the storage enclosure for the three wavelength converters.



Figure 21– Dust proof storage enclosure for the various wavelength converters

Wavelength Separator

There are several ways to separate the wavelengths and point the desired beam in the right direction. We selected to use a pair of Pellin-Broca prisms for minimizing replacing optics at different wavelengths. But the angles of the prisms need to be adjusted to the desired wavelength in order to maintain the beam pointing.

Several different systems were considered and designed for mounting the PB prisms in such a way that they could be rotated accurately to the correct angles. (Figure 22)

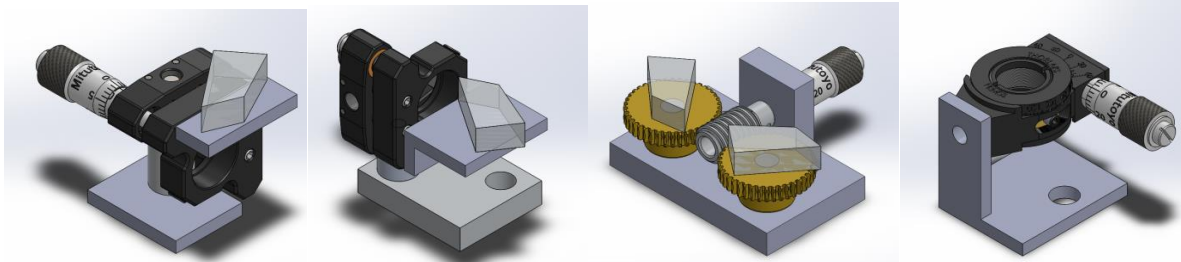


Figure 22–PB Prism mount ideas

A 3D printed model of the final design selection of the PB rotating mount was created (Figure 23)



Figure 23– 3D printed model of PB rotating mount

The final successful implementation is shown in Figure 24.

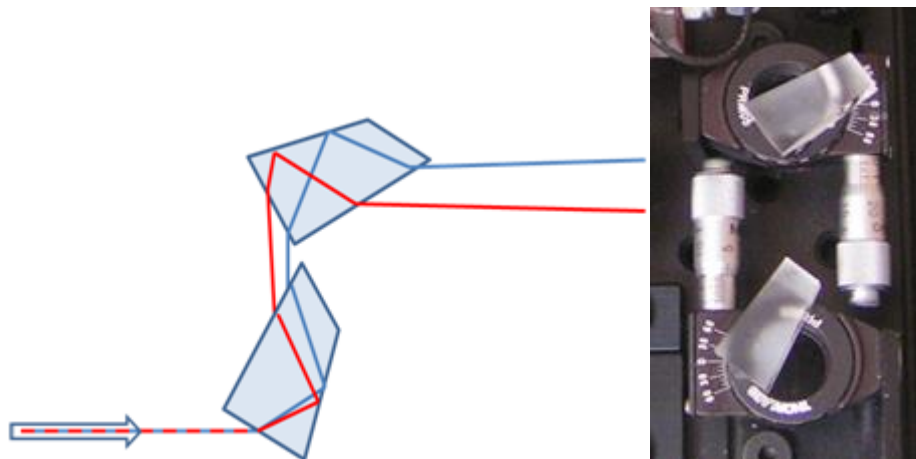


Figure 24– Pellin-Broca prism arrangement for the wavelength separation

Low Cost Design Considerations

The number one goal was low cost. One way that we managed to reduce cost was through the selection of optical components. Multiple vendors were sourced and a cost benefit analysis was performed to find the least expensive option that still meets all of the necessary specifications.

During the component selection process a table was created and constantly update to keep track of the cost, weight, and vendor of all the components for the setup. Cost estimates with price breaks for larger volume orders were also tabulated.

#	Part	Description	Model /manufact	Website Link	Cost	Wt	Detail	Qty	order Total Price	1 off Total Price	LG Qty Total Price
Bread board /Case									\$287.62		
1	Case	Enclosure		http://www.frys.com/product/2090841#del	\$34.99			1	\$34.99	\$34.99	
2	Bread Board	Bread board (8" x 24")	MB824 Thor	http://www.thorlabs.com/thorproduct.cfm	\$239.00		1/4-20 THD	4	\$239.00	\$79.67	
3	Grommett	Rubber mounting gromets	MSC	http://www.mscdirect.com/product/32828	\$16.09		1/4" ID 9/16" OD	100	\$13.63	\$0.41	
Laser Head									\$324.25		
1	Cube Holder	a	Mirror Mount	KM05FL Thor	http://www.thorlabs.com/thorproduct.cfm	\$54.00	0.05		1	\$54.00	\$54.00
		b	Inside ring	63392393 MSC	http://www.mscdirect.com/product/63392	\$3.66		3/8" ID by .5" OD	1	\$3.66	\$0.05
		c	Outside ring	63392419 MSC	http://www.mscdirect.com/product/63392	\$10.57		.5" ID by .75" OD	1	\$10.57	\$0.15
		d	Outside ring 2	63392443 MSC	http://www.mscdirect.com/product/63392	\$14.67		.75" ID by 1" OD	1	\$14.67	\$0.20
		e	Set Screw	67348003 MSC	http://www.mscdirect.com/product/67348	\$13.11		6-32 at 1/4"	1	\$13.11	\$0.13
		f	L-Bracket	6957823 MSC	http://www.thorlabs.com/thorproduct.cfm	\$15.03		1/8" by 1"	1	\$15.03	\$0.31
		g	Plastic riser	63392229 MSC	http://www.mscdirect.com/product/63392	\$6.11		3/8" by 3/8"	1	\$6.11	\$0.08
		h	Post 1/2"	MS05R	http://www.thorlabs.com/thorproduct.cfm	\$5.60	0.01	4-40 thd	1	\$5.60	\$5.60
2	Mounting plates	a	Thread adapter	AP8E4E	http://www.thorlabs.com/thorproduct.cfm	\$1.90	0	8-32 to 4-40	1	\$1.90	\$1.90
		b	Mounting plate small	32000739 MSC	http://www.mscdirect.com/product/32000	\$6.65		3/4" by 1/4"	3	\$19.95	\$0.83
		c	Mounting plate xlarge	Amazon	http://www.amazon.com/gp/product/B000	\$4.24		1.5" by 1/4"	1	\$4.24	\$4.24
		d	Mounting plate thick	Amazon	http://www.amazon.com/gp/product/B000	\$8.64		1.5" by 1/2"	1	\$8.46	\$4.23
3	Mounting screws	a	Mounting plate large	32000747 MSC	http://www.mscdirect.com/product/32000	\$7.38		1" by 1/4"	3	\$22.14	\$4.92
		b	Mounting screw from bottom	MSC	http://www.mscdirect.com/product/05574	\$9.45		4-40 FLAT 3/4"	100	\$9.45	\$2.36
		c	Mounting screws from top	MSC	http://www.mscdirect.com/product/98678	\$12.36		1/4-20 low head	100	\$12.36	\$1.48
		d	Mounting screw from top	MSC	http://www.mscdirect.com/product/98678	\$12.36		1/4-20 low head	100	\$12.36	\$1.48
4	Farady Rotator	a	Outside ring	63392419 MSC	http://www.mscdirect.com/product/633924	\$10.57		.5" ID by .75" OD	1	\$0.15	\$0.15
		b	Set Screw	67348003 MSC	http://www.mscdirect.com/product/67348	\$13.11		6-32 at 1/4"	1	\$0.13	\$0.13
5	Cube Holder 2	a	Mirror Mount	KM05FL Thor	http://www.thorlabs.com/thorproduct.cfm	\$54.00	0.05		1	\$54.00	\$54.00
		b	L-Bracket	6957823 MSC	http://www.mscdirect.com/product/06957	\$15.03		1/8" by 1"	1	\$0.31	\$0.31
		c	Plastic riser	63392229 MSC	http://www.mscdirect.com/product/63392	\$6.11		3/8" by 3/8"	1	\$0.08	\$0.08
		d	Post	MS05R	http://www.thorlabs.com/thorproduct.cfm	\$5.60	0.01	4-40 thd	1	\$5.60	\$5.60
		e	Thread adapter	AP8E4E	http://www.thorlabs.com/thorproduct.cfm	\$1.90	0	8-32 to 4-40	1	\$1.90	\$1.90
7	Turning Mirror	a	Mirror Mount	KM05FL Thor	http://www.thorlabs.com/thorproduct.cfm	\$54.00	0.05		1	\$54.00	\$54.00
		b	Post	MS05R	http://www.thorlabs.com/thorproduct.cfm	\$5.60	0.01	4-40 thd	1	\$5.60	\$5.60
		c	Thread adapter	AP8E4E	http://www.thorlabs.com/thorproduct.cfm	\$1.90	0	8-32 to 4-40	1	\$1.90	\$1.90

Table 1– Optical component spreadsheet comparison list

One way that was found to reduce cost, weight and size was to design and fabricate custom mounting plates for the optics. (Figure 25)

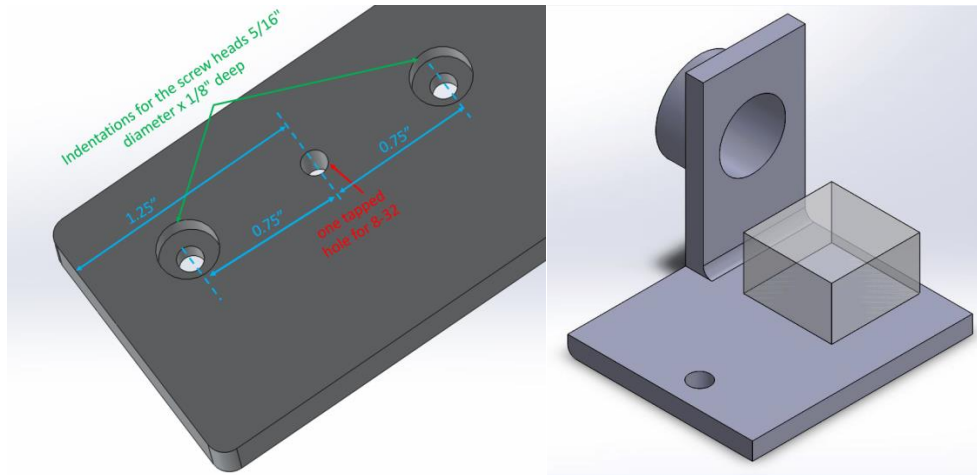


Figure 25– CAD model of custom mounting

An enclosure was selected and designed for the breadboard layout. This was again modeled in SolidWorks. Along with the enclosure, an anti-vibration system was designed for the case using rubber grommets. (Figure26)

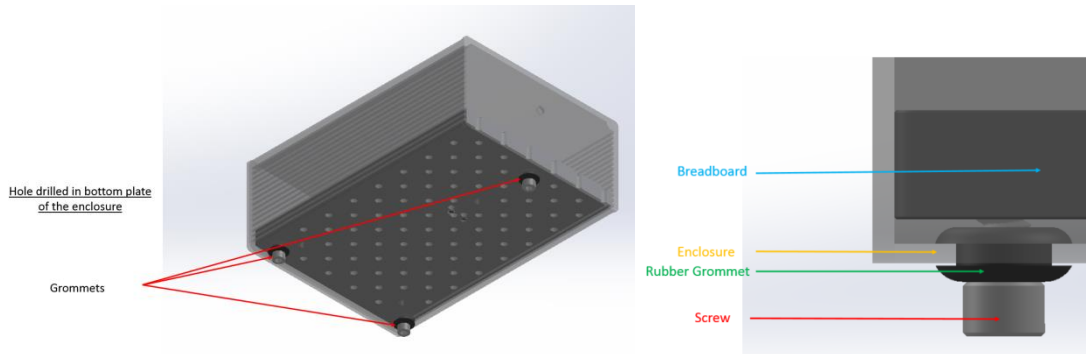


Figure 26– CAD model of case with grommets

Another way to keep the cost low was to research the most cost effective methods for fabrication of components. Larger volume runs for machining and anodizing lead to large cost savings per part in the long run.

Before having parts fabricated, a 3D model was printed to verify dimensions and clearances. (Figure 27) These parts were assembled on the breadboard to verify clearance and fit.

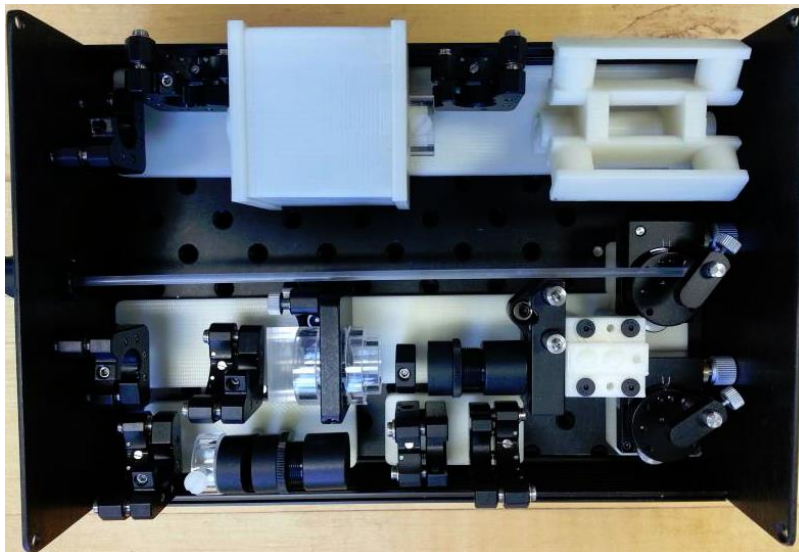


Figure 27– 3D model

After mocking up the system with the 3D parts, any modifications that were needed were then updated in the SolidWorks model. This process of drawing modifications followed by a 3D mockup was repeated several times before converging on a final design with correct dimensions. (Figure 28)

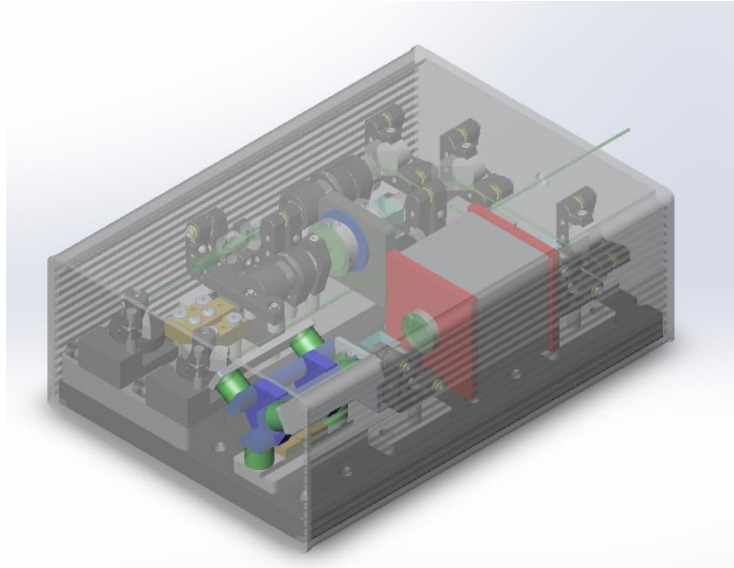


Figure 28– CAD model of breadboard and case assembly

Once this final design was updated for the SolidWorks model, all of the individual parts files that need to be fabricated were transformed into 2D CAD files. (Figure 29)

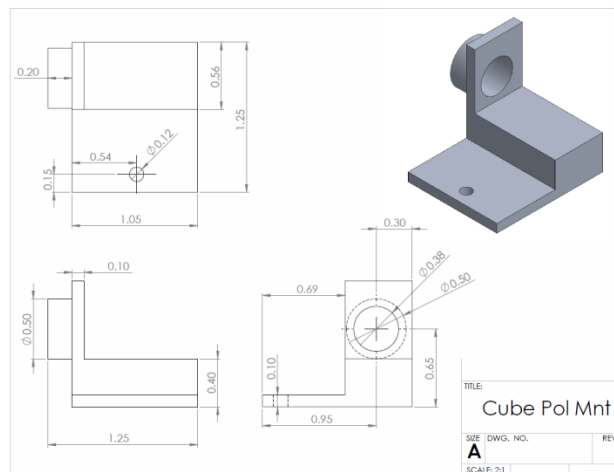


Figure 29– 2D CAD drawing of part to be fabricated

These drawing files were then sent over to the machine shop where the parts were created using the correct materials (aluminum for the majority of parts). These parts were then mounted to the bread board just as the 3D printed parts had been, and again double checked for clearance fit and positioning. (Figure 30)



Figure 30 – Machined components

After any modifications were done to these parts and the final version was converged upon, the parts were then sent off to be anodized. The final anodized parts were assembled back on the bread board. (Figure 31)

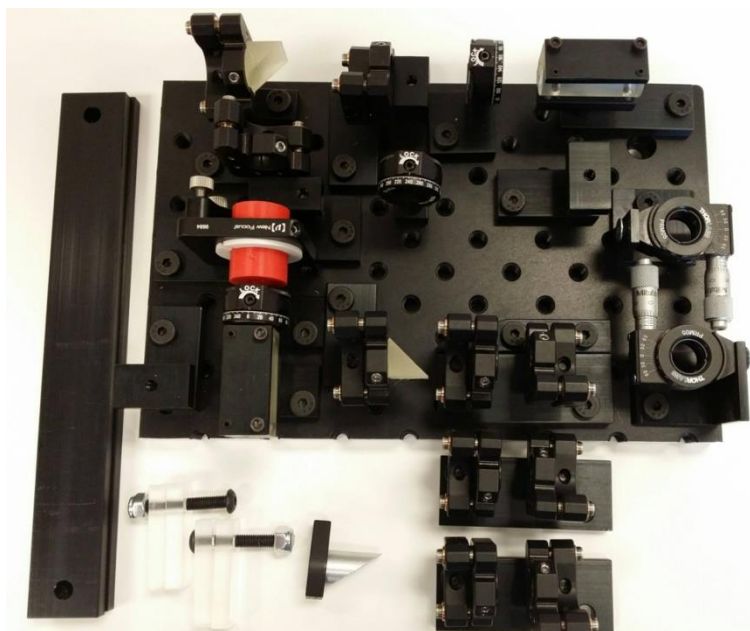


Figure 31– Anodized Parts assembled on breadboard

Another way to reduce costs, along with saving weight and space, was in the creation of custom parts. It was found that in several cases this proved to be cheaper and more efficient than purchasing an existing off the shelf product that may still need to be modified. One of these custom pieces was the laser rod mount design, which was first designed in SolidWorks. (Figure 32)

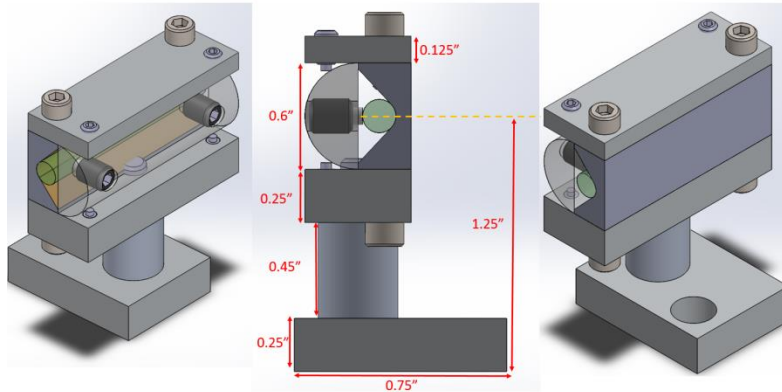


Figure 32 – Custom designed laser rod mount

As new parts were designed and added, and old parts were modified, the overall system assembly was continuously updated to reflect these revisions. (Figure 33)

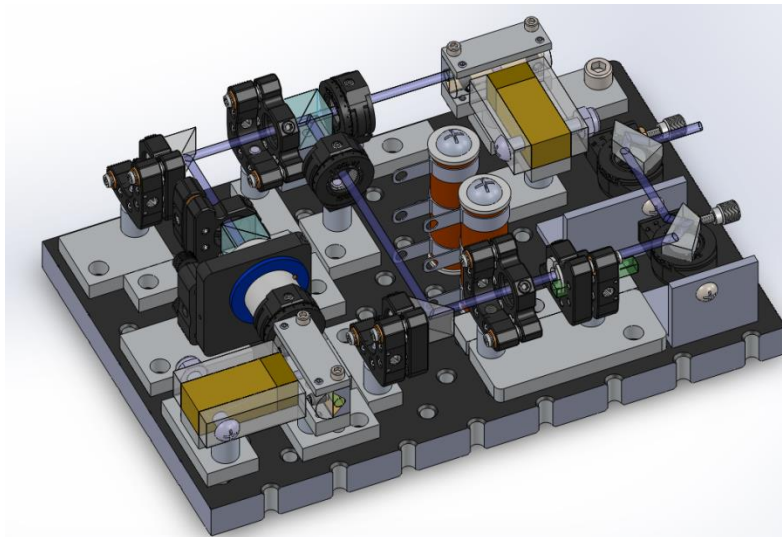


Figure 33 – SolidWorks model of new system design

After the new version of the system was completed in SolidWorks, the parts were then sent to the 3D printer and a mockup was assembled using these parts. (Figure 34)

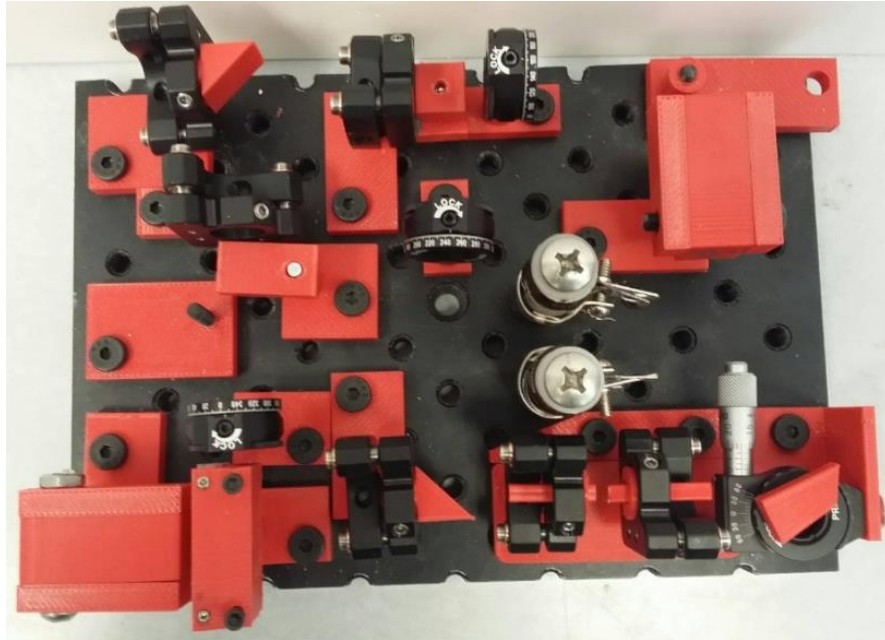


Figure 34 – System layout mockup using 3D printed components

After the clearance and fit of the parts were verified with the 3D print parts mock up, the next step was to send the drawings of these parts to the machine shop to be fabricated. Many of these parts would also need to be anodized as well. A layout of the parts that were to be anodized was created in SolidWorks. (Figure 35, 36)

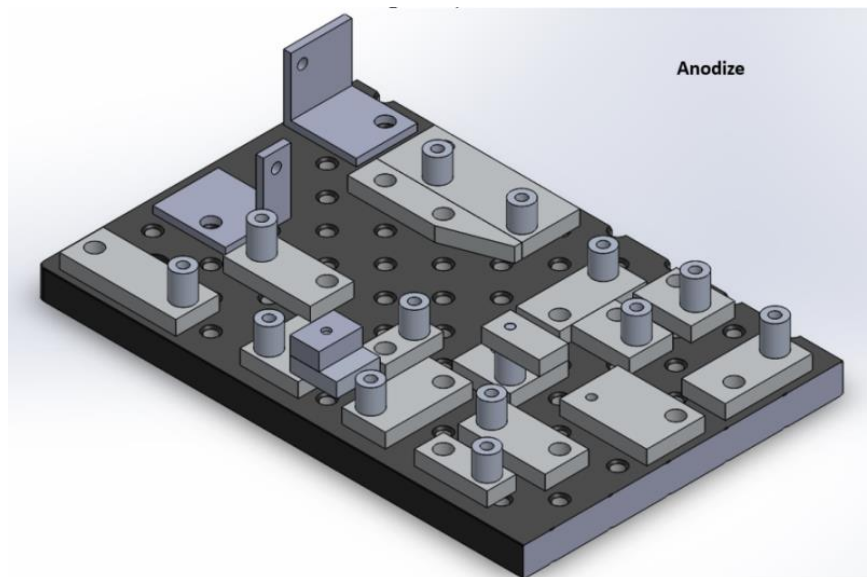


Figure 35 – Parts to be anodized

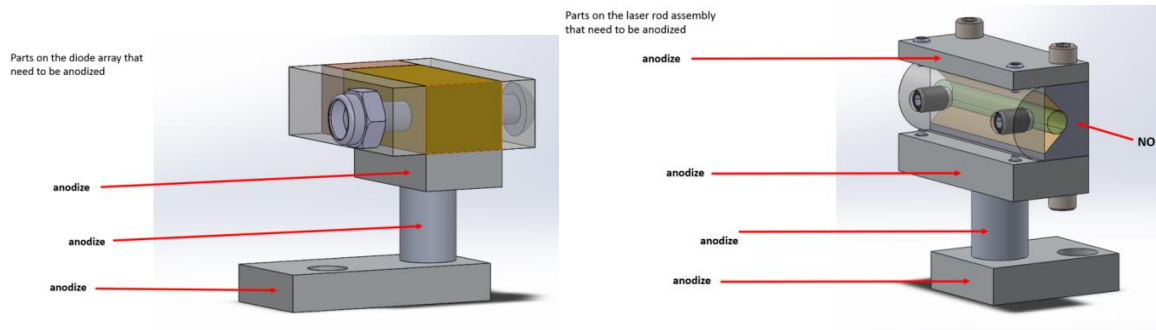


Figure 36 – Parts to be anodized

After several further modifications and adjustments to the layout design, mounts and components, multiple boards were populated with anodized parts. (Figure 37)

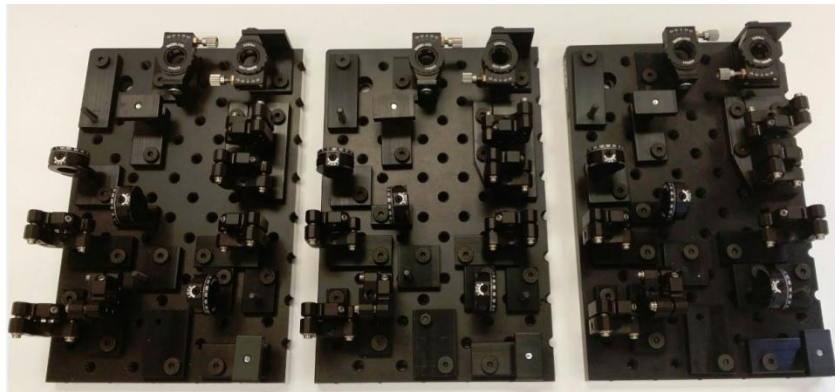


Figure 37 – Multiple boards populated with anodized parts

These boards were then fitted into the rubber mounted packaging cases (Figure 38)



Figure 38 –Populated with anodized parts mounted in enclosure

Compact Low Cost Laser Driver

The laser driver contains: 1) An internal pulse oscillator for generating 1Hz, 10 Hz, and 100Hz. 2) A pulse width modulator to vary the drive pulse duration which control the laser output pulse energy. 3) A high current electronic switch to drive the diode arrays. 4) A trigger pulse for the Q-switch driver. 5) A push button to activate the laser. 6) A trigger IN and a trigger OUT for synchronizing with other detection equipment. Figure 39 shows the block diagram of the laser driver.

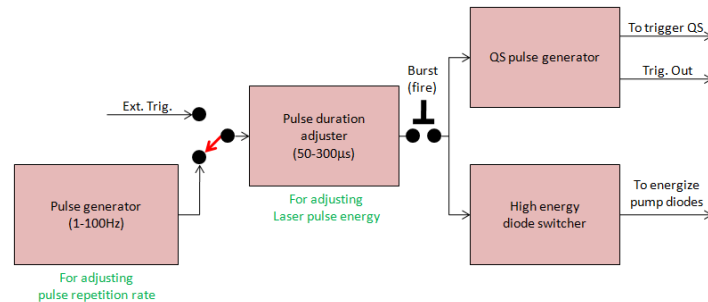


Figure 39– Block diagram of the laser driver

We developed and successfully tested a laser driver for burst mode operation. Commercial drivers are designed and built for continuous operation and not burst mode. Therefore, they are larger and very expensive. Our driver is extremely inexpensive. The material cost is under \$50 and it can be packaged into a 1.5" x 2" x 5" enclosure. It contains the power supply and drive electronics. It also contains a trigger to automatically trigger the Q-switch and trigger IN and trigger OUT for synchronizing with a detection system. Figure 40 shows the driver and the current pulse it generates to drive the entire set of diodes used in the laser system.

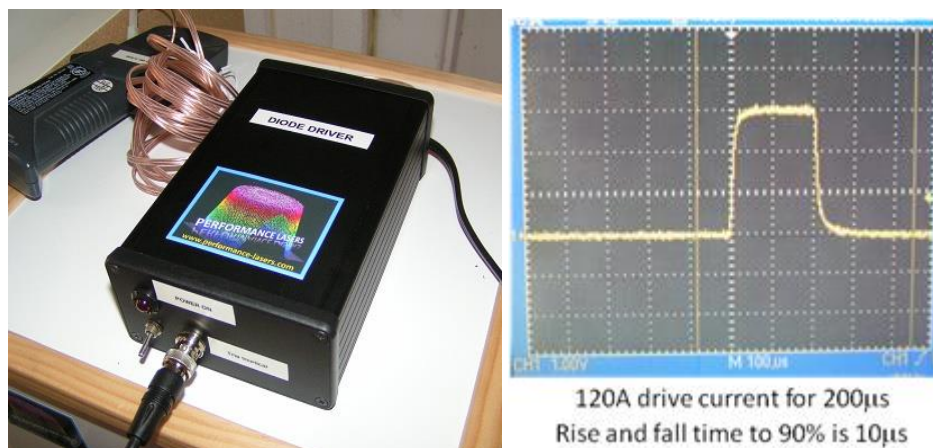


Figure 40 – Extremely compact and low cost laser driver (includes power supply, diode driver, and Q-switch trigger) and its current pulse

The drive electronics is capable of delivering up to 500A peak current. The driver was tested under all of the required burst modes conditions and is currently used to drive the laser system.

Low Cost Q-Switch Driver

A commercial Q-switch driver costs nearly \$2,000. We had to reduce the cost of the Q-switch driver to meet the goal requirements. We designed a new circuit and constructed it. Figure 41 shows the new compact Q-switch driver.

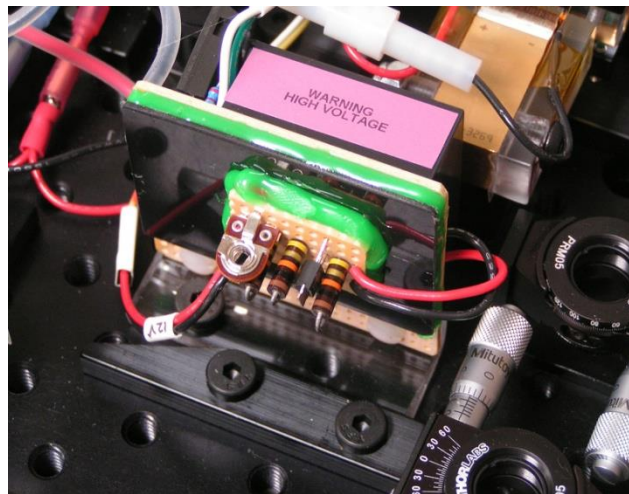


Figure 41 – Extremely compact and low cost Q-switch driver

The material cost of the driver is under \$150 which is about 1/10 of the cost of a commercial driver. We did not have a single failure of the new Q-switch driver.

Battery / Inverter Pack

The power consumption of the burst laser is about 2W for 1Hz continuous operation, and about 20W at 10Hz burst. During the OFF time between bursts, the power consumption is only few mW. Therefore, the average power consumption is very low.

Since the average power required is low. A battery can be used to run the laser for autonomous field operation or on small robotic vehicles. In order to widen the potential applications of the laser system, 12Vdc would be the preferred choice since most vehicles has 12V battery. A rechargeable 12V polymer Li-ion battery pack was constructed to power the laser system. An inverter to convert the 12Vdc to 115Vac is used; therefore, plugging the laser power cord to the inverter instead of the wall plug enables us to use the laser system in the field.

A case for external battery power supply needed to be designed and built. This case needed to be low cost, lightweight, portable, suitable for outdoor applications and easy to carry. An initial design was created in SolidWorks for an insert to hold the batteries, inverter and wiring in place inside of a rugged off the shelf carrying case. (Figure 42, 43)

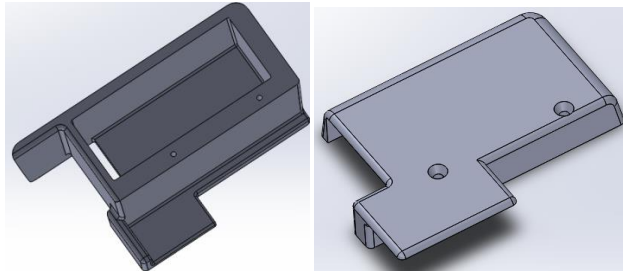


Figure 42 –SolidWorks model design for battery case insert

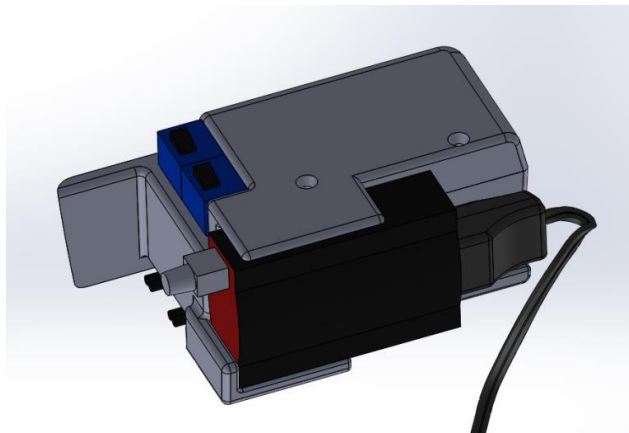


Figure 43 –SolidWorks model assembly for battery case insert

After the SolidWorks design was revised and finalized the model was then converted to the appropriate file type and sent to the 3D printer. This 3D insert was installed in the Pelican case along with the batteries, inverter and wiring. (Figure 44)



Figure 44 – Polymer Li-ion battery for powering the burst laser system

Complete Systems

A photograph of the complete system is shown in figure 45. It contains the laser module, the laser driver unit that plugs to 115Vac and the wavelength converters that can be inserted into the laser module for operating at 1570nm, 355nm, or 266nm.



Figure 45 – Complete laser system (laser module in center, laser driver on left, and wavelength converters on right)

The laser system and battery pack are housed in a small briefcase (18"x13"x6") for easy transportation and storage. (Figure 46)



Figure 46 – Burst laser in a briefcase

Figure 47 shows the fully completed three prototypes burst lasers in their briefcases.



Figure 47 – Three completed prototype burst lasers in their briefcases

Manual

A manual like the one shown in figure 48 for powering and operating the burst laser is attached to each of the laser systems. The burst laser is maintenance free and the operator should not attempt to troubleshoot or repair the laser system.

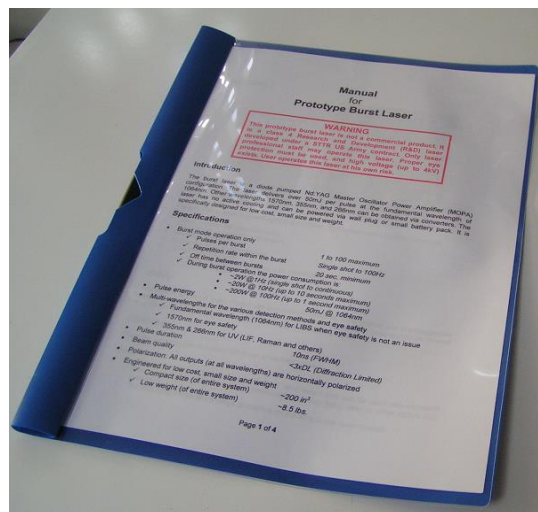


Figure 48– Operator manual for the prototype burst laser

Cost Estimates

The cost to produce the burst laser is the number one goal. We have made every effort to minimize the cost of the system. We were able to build a laser system for a total material cost of about \$5,500 (not including wavelength converters and battery pack). The options for wavelength converters, wavelength separator, and battery pack will add to the material cost about \$2,000. High volume production should reduce the material cost at minimum by 25% and possibly by over 50%. Therefore, the selling price per unit at high volume may well be under \$8,000.

Estimates of Technical Feasibility

The final goal is to have low cost and compact commercial burst lasers to be integrated in CBRNE detection applications. Phase II clearly demonstrated the feasibility of clearing the way toward commercial systems that meet the desired low cost, size and weight. With the design and component selection of this prototype it was possible to reduce the cost as compared to the present readily available lasers on the market that have comparable specifications.

The prototype laser has been designed to be used indoor and in outdoor field scenarios. The size and weight was optimized so that the laser and battery pack could easily and comfortably be carried. The packaging was also designed to be rugged and to reduce vibrations.

All that is left to do is: 1) add temperature control to expand the current range of 70F – 80F to a wider range if needed, 2) control the laser remotely via WiFi, Blue Tooth, etc. with smart phone if needed, 3) add safety features like interlocks, warning lights, etc. if needed, 4) do reliability, shake and bake testing, and 5) engineer it for mass production.

The transition time to mass production will vary on the added requirements, but should take as low as one year and up to three years at the most.